MIDMARK®

Installation/Operation Instructions

9A78001 VISION BLOCK SCREEN

KIT COMPONENTS

Part Number	Description	Qty.
9A78001	Vision Block Screen	1
003-0935-00	Installation / Operation Instructions	1

REQUIRED TOOLS

None

INTRODUCTION

To obscure patient's vision of a general procedure / examination.

WARNING

Only mount 9A78001 on base rail of exam table or side rail of stretcher. Assure table or stretcher is clear of any obstacles that may interfere with operation of Vision Screen.

INSTALLATION

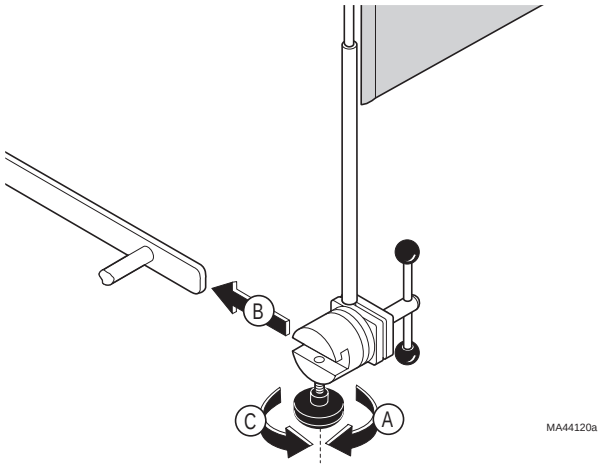

A. Loosen lower knob on swivel block
B. Slide swivel block onto exam table *base rail* or stretcher side rail.
C. Position at desired location and tighten knob.

OPERATION

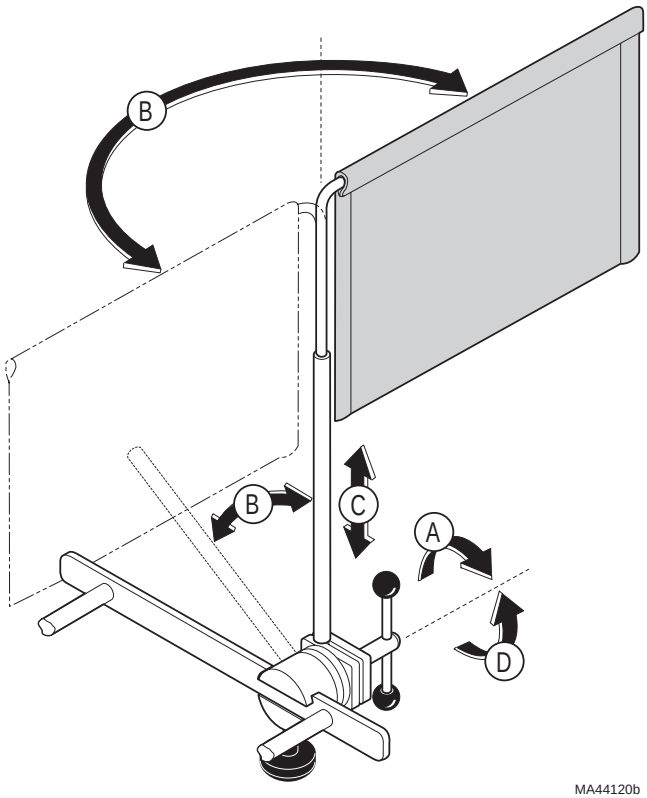

A. Supporting Vision Block Screen, loosen T-handle.
B. Rotate Screen to desired position.
C. Position Screen at desired height.
D. Tighten T-handle.

© Midmark Corporation - 1998